

While we are waiting to start

- Please, so that we may get to know you, our audience a little better and for CME
- Please use your chat box
 - Enter your name and email address (for CME)
 - Enter your role in patient care (doctor, nurse, technician, RT, MA, etc)
 - Enter your comfort level with spirometry on a scale of 1-5 with:
 - 1 = Not very comfortable with spirometry
 - 5 = Very comfortable with spirometry

Reviewing the 2017 ATS Updates to the 2005 ATS/ERS Guidelines: How to Perform, Interpret & Report Spirometry

Seminar # 3701

James M. Quinn, MD, FACP, FAAAAI

Associate Professor of Medicine, Uniformed Services University of the Health Sciences
Associate Adjunct Professor of Medicine, University of Texas Health Science Center San Antonio
San Antonio Uniformed Services Health Education Consortium, Wilford Hall Ambulatory Surgical Center

Karla E. Adams, MD, FAAP, FACAAI

Associate Professor of Pediatrics, Uniformed Services University of the Health Sciences
San Antonio Uniformed Services Health Education Consortium, Wilford Hall Ambulatory Surgical Center

Disclosures

- No disclosures
- The views expressed are those of the presenter and do not reflect the official views or policy of the Department of Defense or its components

Learning Objectives

- Identify the source and relevance of the ATS/ERS guidelines for lung function testing and reporting
- Discuss the ATS/ERS recommendations for correct performance and reporting of spirometry
- Identify ATS/ERS guidelines to interpret and classify the severity of identified abnormalities

Sources

- ATS/ERS sources
 - Standardization of Spirometry 2019 Update - American Journal of Respiratory & Critical Care Medicine, Vol 200, 2019, 70-88.
 - Recommendations for a Standardized Pulmonary Function Report—American Journal of Respiratory & Critical Care Medicine, Vol 196, 2017, 1463-1472.
 - General considerations for lung function testing - European Respiratory Journal, Vol 26 (1), July 2005, pp 153-161
 - Standardisation of spirometry - European Respiratory Journal, Vol 26 (2), August 2005, pp 319-338
 - Interpretive strategies for lung function testing - European Respiratory Journal, Vol 26 (5), November 2005, pp 948-968.
 - ATS website = <https://www.thoracic.org/statements/pulmonary-function.php>

Overview

- Background
- Spirometry and ATS/ERS guidance
 - Performance of test – new 2019
 - Interpretation
 - Assessment of normal – new 2017 & 2019
 - Reference pools – new 2017
 - Determining adequacy – new 2017 & 2019
 - Approach to evaluation
 - Severity classification



Instrumentation

- Spirometer
 - Meets standards of ISO 26782 reviewed 2016



Instrumentation

- Spirometer
 - Meets standards of ISO 26782 reviewed 2016
 - Flow-volume and volume-time displays explicitly required

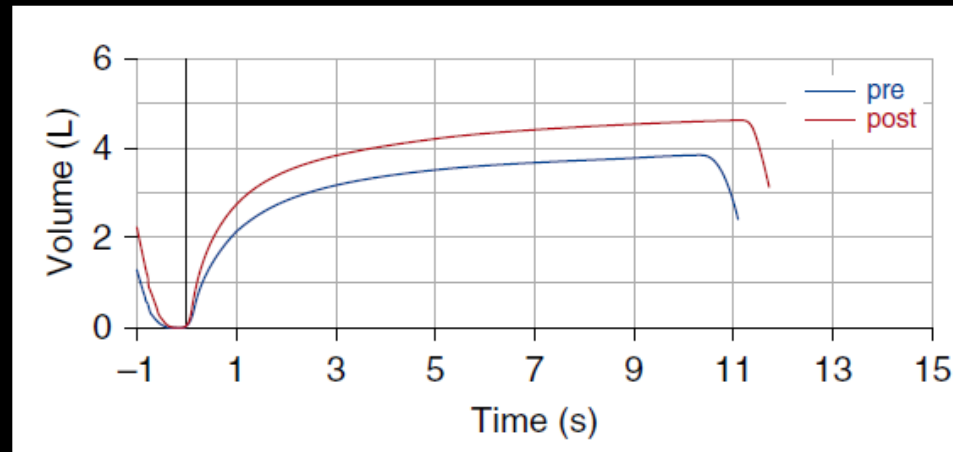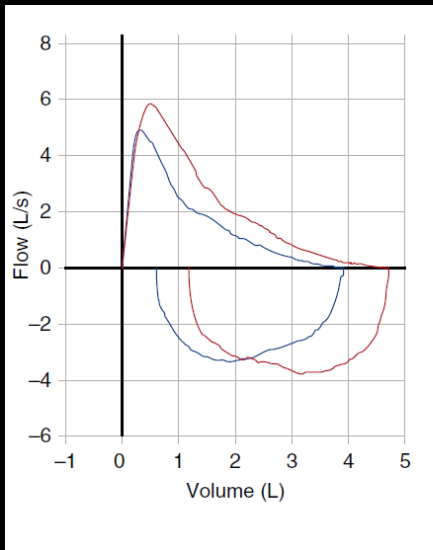

Instrumentation

- Spirometer
 - Meets standards of ISO 26782 reviewed 2016
 - Flow-volume and volume-time displays explicitly required
- 3 L calibration syringe for daily calibration



Performing Spirometry

- Preparatory instructions
 - Avoid smoking within 1 hour
 - Avoid alcohol/intoxicants within ~~4 hours~~ 8 hours
 - Avoid vigorous exercise within ~~30 min~~ 1 hour
 - Avoid constricting clothing of chest/abdomen
 - Avoid loose fitting dentures
- Prepare the subject
 - Ask about illness, pain, smoking, medication, etc
 - Measure standing height and weight
- Explain and demonstrate the test

Eur Respir J 2005;26:319-38.

Am J Respir Crit Care Med 2019;200:70-88.

Performing Spirometry

- Wash hands – operator and patient
- Quiet comfortable environment (drinking water, tissues)
- Patient in correct posture
 - Seated erect
 - Shoulders slightly back, chin elevated
 - Seated in chair with arms, without wheels, feet flat on floor
- Attach nose clips
- Ensure tight seal of mouth on mouthpiece (generally behind the teeth and on top of tongue)
- A well-trained, well-motivated, enthusiastic nurse or technologist is key

Performing Spirometry in COVID19 Era

- Screen patients acknowledging difficulties
- Limit tests to essential for immediate treatment decisions
- Reassess risk/benefits over time
- Measures to protect staff and patients
 - PPE that limits aerosolized droplet acquisition in accord with your infection control team
 - Gowns
 - Gloves
 - N-95
 - Face shield or googles
 - Enhanced cleaning, wiping down surfaces with appropriate cleansers
 - Negative pressure room if available (it is not for us)
 - Determine room air exchange to assess dormant interval between tests (1 hour for us)

Performing Spirometry



Performing Spirometry

- Forced Vital Capacity Maneuver
 - From a maximal inspiration, the maximal volume of air exhaled with maximally forced effort
 - 4 distinct phases
 1. Maximal inspiration – **largest source of error** is inadequate maximal inspiration
 2. “Blast” of exhalation
 3. End of forced expiration (no volume change = plateau = <0.025 L over 1 sec) but no longer than 15 seconds – **second largest source of error** is ending prematurely
 4. **Inspiration at maximal flow back to maximal lung volume**

Performing Spirometry

- Exhale maximally and completely until no more air can be expelled (maintain posture)
- Use “vigorous” coaching (warn patient)
 - “Blast it out !!!” as opposed to “blow”
 - “Keep going, keep going !!!”, “More, more, more !!!”
 - “Squeeze it out ... until your lungs are completely empty”
- There is no longer a minimum requirement for FET (previously 6 sec – adult; 3 sec – child)

Performing Spirometry



- Inspire with maximal effort until completely full
 - “Completely fill your lungs back up”
- Perform minimum of 3 maneuvers
 - No more than 8 are usually required
 - Except children may benefit from more than 8

Most Common Errors

- Patient
 - Failure to take a complete inhalation prior to exhalation
 - Stops exhaling too soon
 - Slow test start = didn't "blast" out at beginning of test
 - Obstructed mouthpiece with teeth or tongue
 - Cough during test
- Technologist
 - Failure to request enough efforts to obtain best effort
 - Insufficient motivation & enthusiasm to obtain best effort

Clinical Data Gathered


- Forced Vital Capacity (FVC) maneuver
- Graphic displays
 - Flow Volume Loop – single best effort
 - Volume vs time curve – single best effort

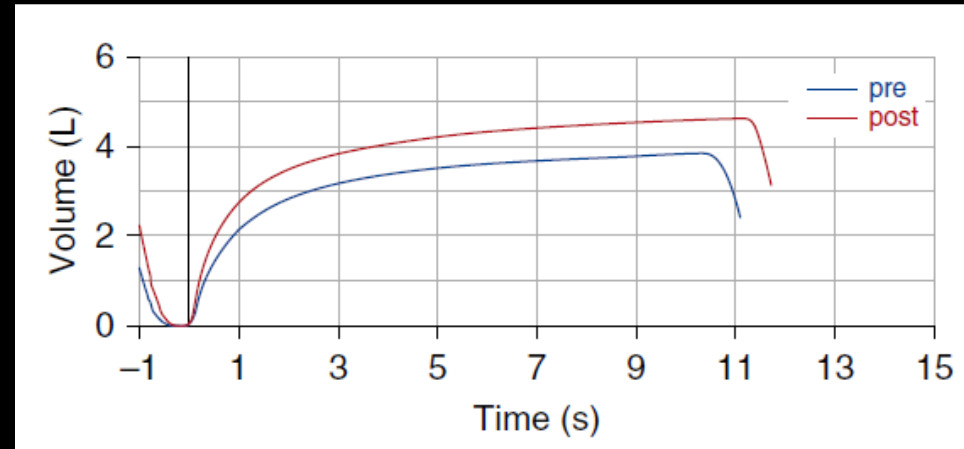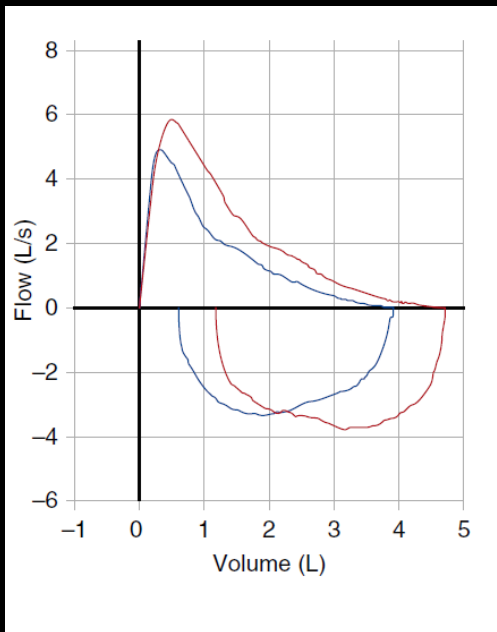


Flow-Volume Loops

- Recognize characteristic patterns
- Recognize poor effort or mistakes
- Directly determine peak flow
- Directly determine FVC

Flow-Volume Loop

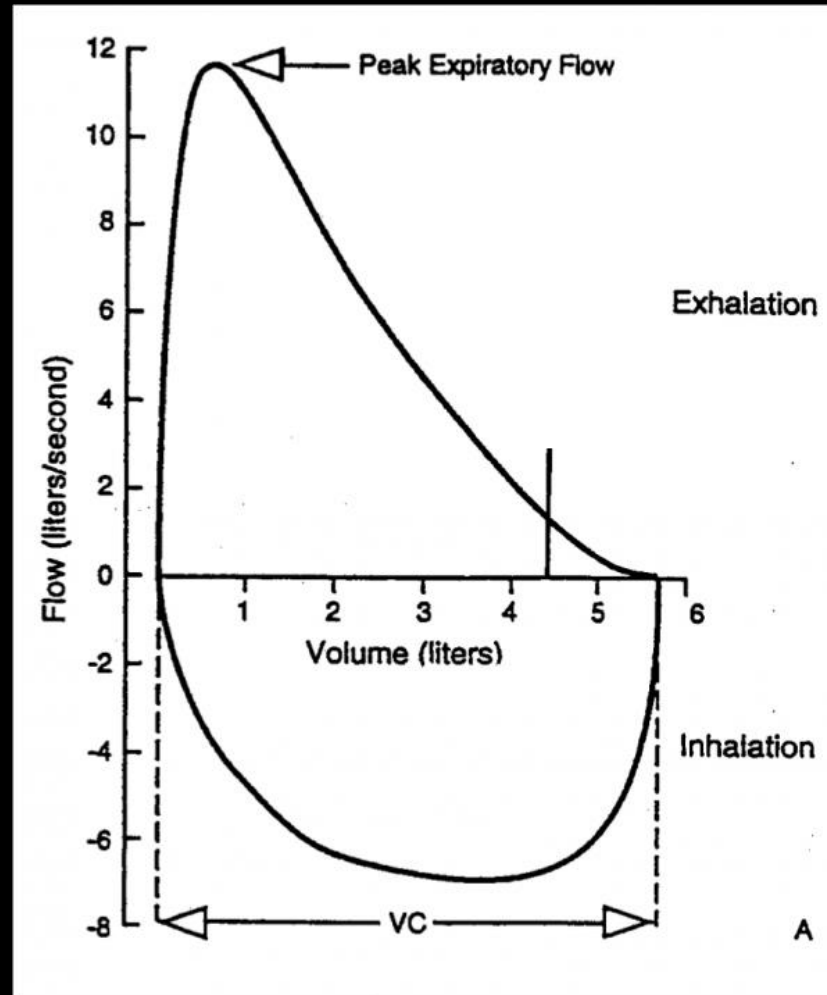

Flow-Volume Loops: Patterns

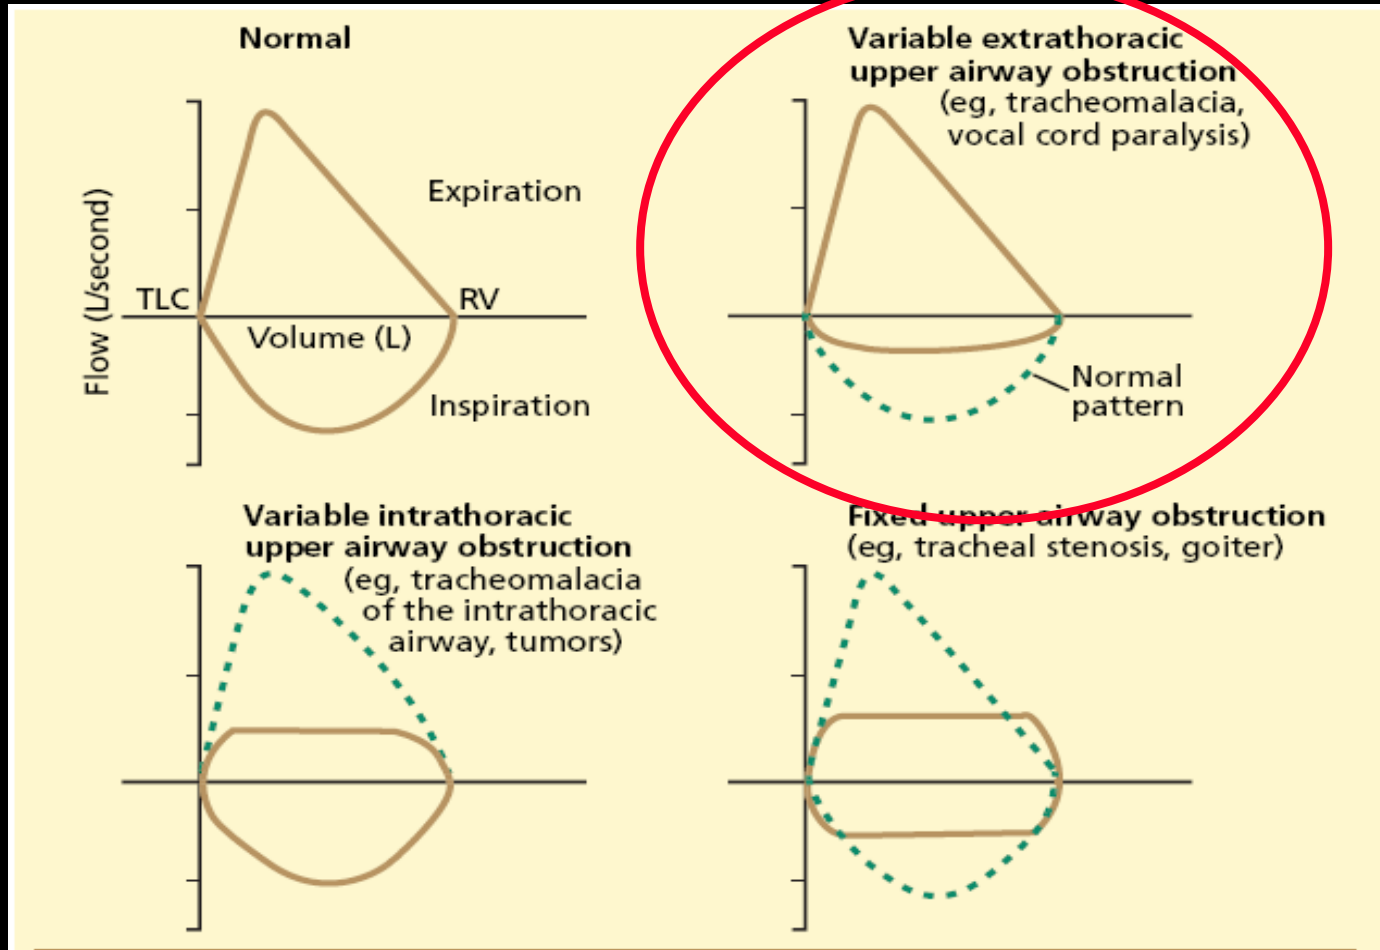


Volume vs Time Curve

- Recognize characteristic patterns
- Recognize poor effort or mistakes and when they occur during the maneuver
- Directly determine FEV1
- Directly determine total expiratory time (TET)
- Directly determine FVC

Volume vs Time Curve

The Volume–Time Curve (The Spirogram)

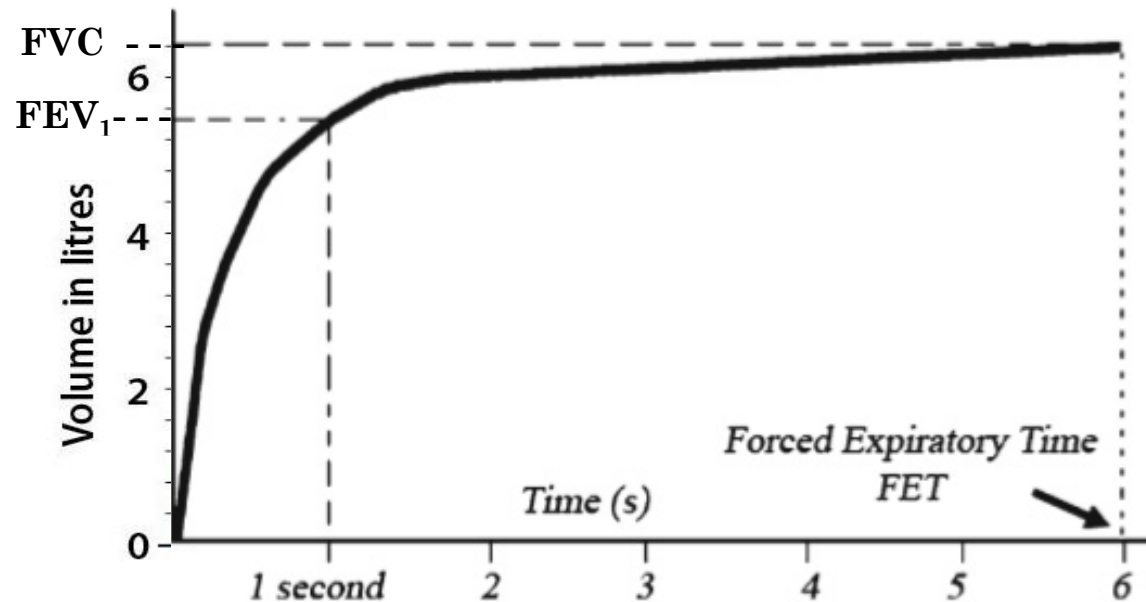



Allergy & Immunology Clinic
Wilford Hall Ambulatory Surgical Center
1100 Wilford Hall Loop
San Antonio, TX 78236 Phone: (210) 292-4278

Patient

Name: Cough Test

ID: 10001

Test date/time: 2/17/2019 7:33:03 PM

Height at test: 66 in

Weight at test: 160 lb

BMI at test: 25.9

Physician: Doctor D. Doctor, M.D.

Predicted set: GLI 2012

Sex: M

Birthdate: 01-Jul-62

Age at test: 56



Smoking history (pk-yr): N/A

Ethnicity: White

Technician: James M. Quinn, MD

Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.44	3.18	-1.20	83	
FEV ₁	L	2.73	2.49	-1.14	84	
FEV ₁ / FVC	%	79	67	0.04	100	
FEF ₂₅₋₇₅ [ISO]	L/s	2.23	1.46		77	
PEFR	L/s	8.48	6.54		98	
FET	sec	8.72				

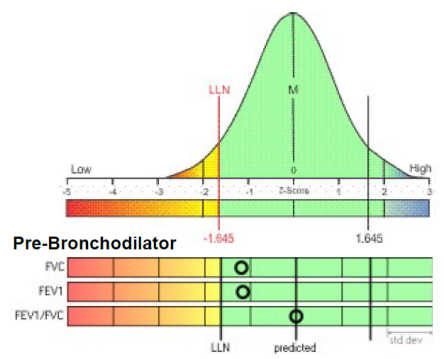
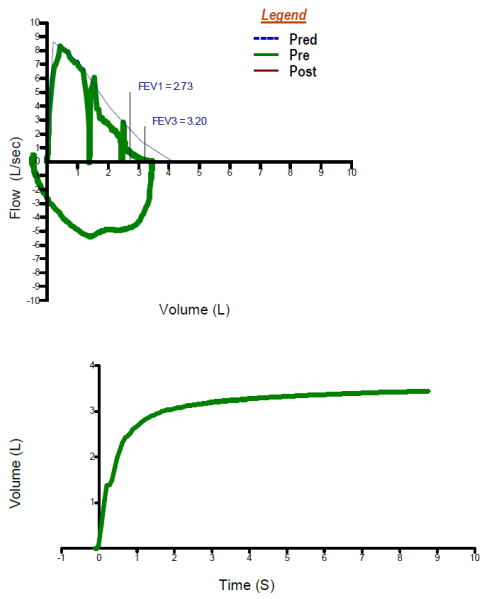


Meets ATS Effort



Meets ATS Reproducibility

Summary of all Pre Efforts

	Pred	Best	%Prd	1	2	3	4	5	6	7	8
StartTime				19:33	19:35	19:36	---	---	---	---	---
FVC	L	4.14	3.44	83	3.44	3.36	3.25	---	---	---	---
FEV ₁	L	3.26	2.73	84	2.68	2.73	2.70	---	---	---	---
FEV ₁ / FVC	%	79	79	100	78	81	83	---	---	---	---
FET	sec	---	8.72		8.72	8.48	7.42	---	---	---	---
V [EXT]	L	---	0.10		0.10	0.05	1.07	---	---	---	---
V [EXT]/FVC	---	---	---		---	---	---	---	---	---	---
⊗ Fails ATS due to:				Start of expiration	Start of expiration	Cough					

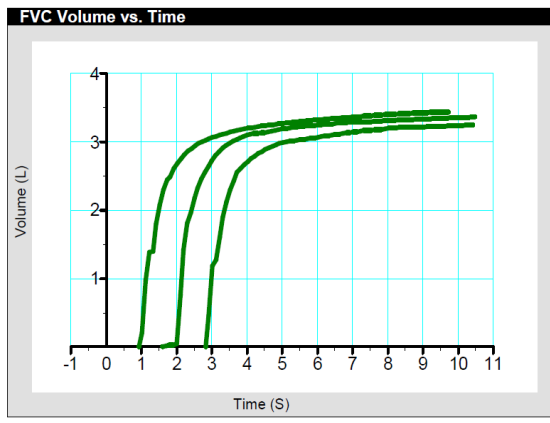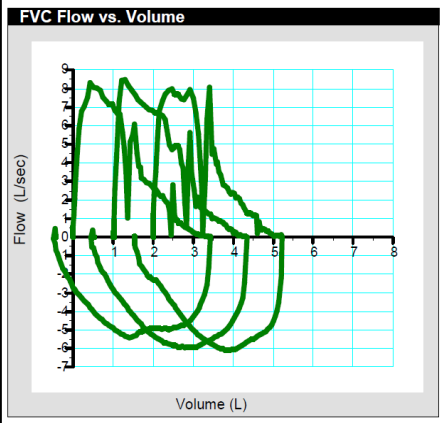

Cough in First Second
Delete Curve; Correction: Try a drink of water

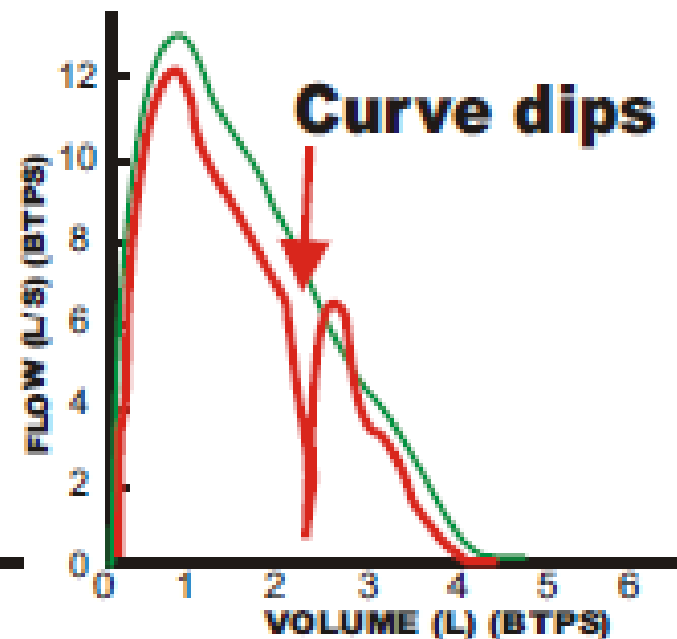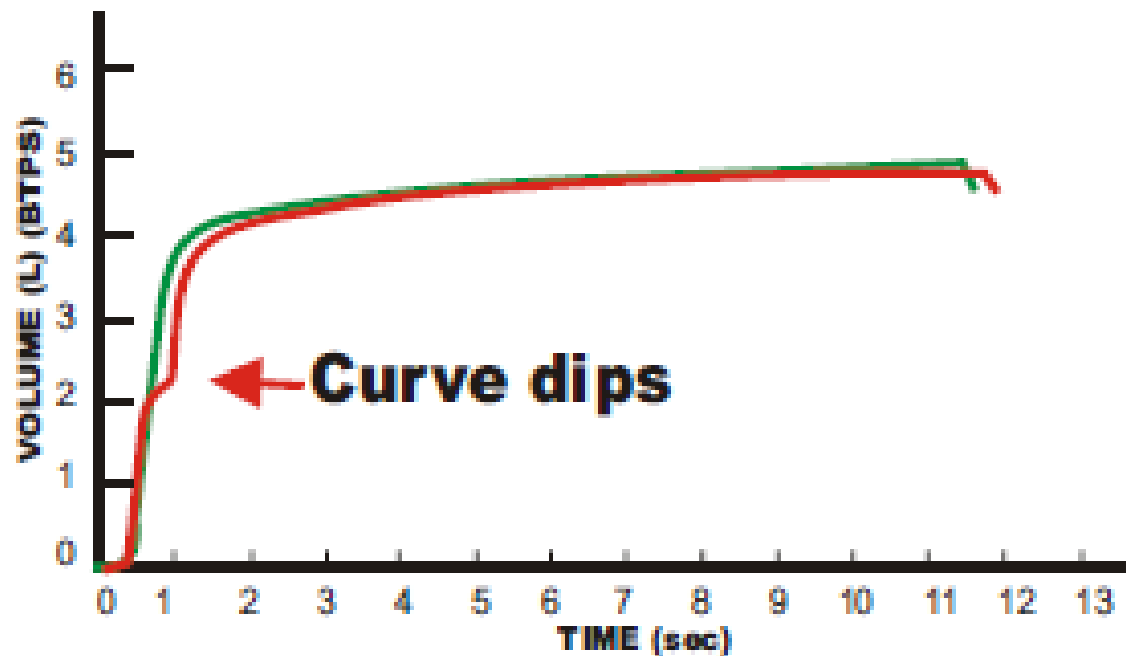

Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236 Phone: (210) 292-4278

Patient

Name: Earlterm Test

ID: 10002

Test date/time: 2/17/2019 7:54:30 PM

Height at test: 66 in

Sex: M

Birthdate: 01-Jul-62

Age at test: 56

BMI at test: 25.9


Smoking history (pk-yrs): N/A




Ethnicity: White

Technician: James M. Quinn, MD

Predicted set: GLI 2012

Spirometry

Spirometry					ATS 	
Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	2.79	3.18	-2.33	67	
FEV ₁	L	2.77	2.49	-1.05	85	
FEV ₁ / FVC	%	99	67	3.49	125	
FEF ₂₅₋₇₅ [ISO]	L/s	4.77	1.46		165	
PEFR	L/s	8.21	6.54		95	
FET	sec	0.78				

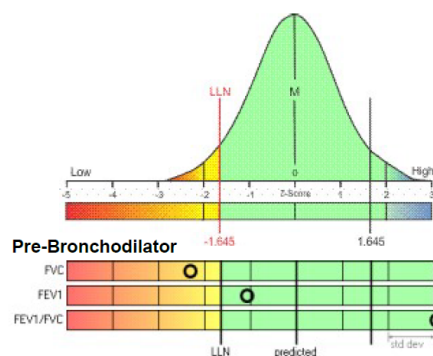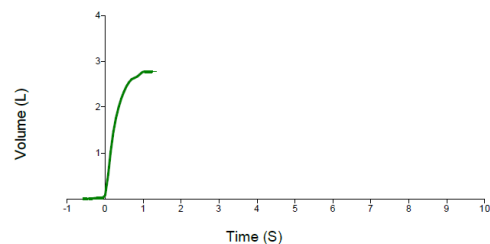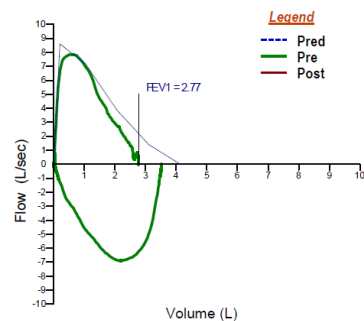

Summary of all Pre Efforts

[illegible]


 Fails ATS due to:

Start of
expiration


Start of
expiration

Start of
expiration



FVC Flow vs. Volume

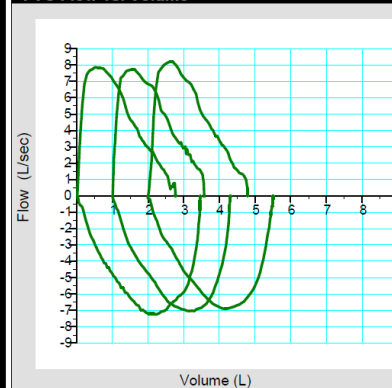

FVC Volume vs. Time

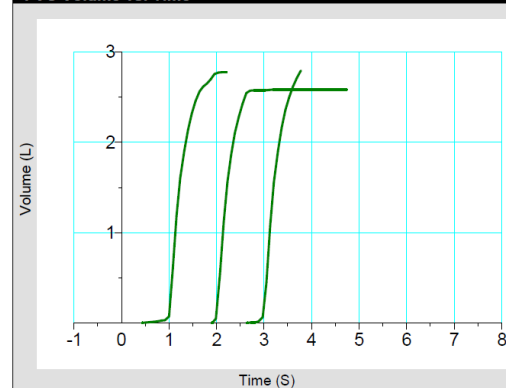

No Plateau Before 15 Seconds
Coach: Keep blowing until told to stop

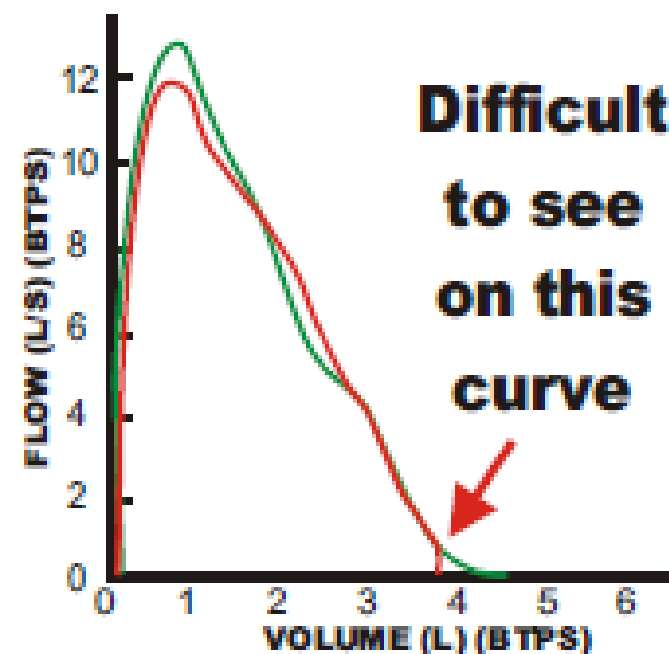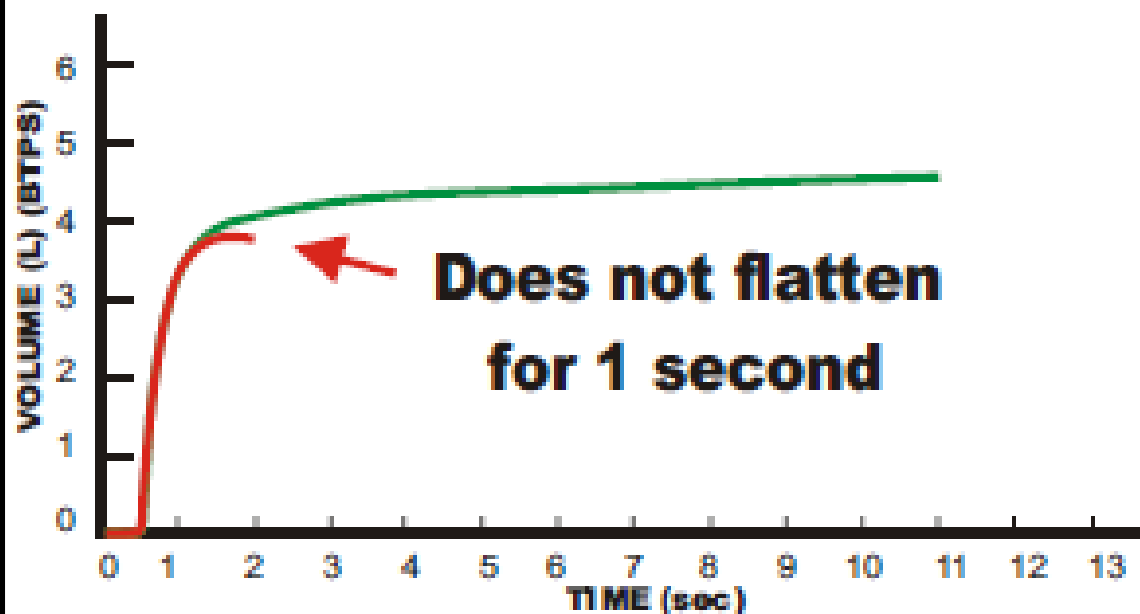



Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236



Phone: (210) 292-4278

Patient


Name: Hesitation Test **ID:** 10003 **Test date/time:** 2/17/2019 8:11:49 PM
Height at test: 66 in **Sex:** M **Birthdate:** 01-Jul-62 **Age at test:** 56
Weight at test: 160 lb **Smoking history (pk-yrs):** N/A **Ethnicity:** White
BMI at test: 25.9 **Physician:** Doctor D. Doctor, M.D. **Technician:** James M. Quinn, MD
Predicted set: GLI 2012

Spirometry


Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.61	3.18	-0.90	87	
FEV ₁	L	3.04	2.49	-0.47	93	
FEV ₁ / FVC	%	84	67	0.83	106	
FEF ₂₅₋₇₅ [ISO]	L/s	3.75	1.46		130	
PEFR	L/s	7.52	6.54		87	
FET	sec	8.47				

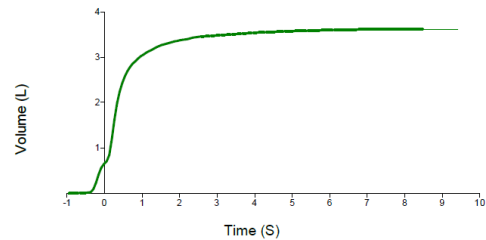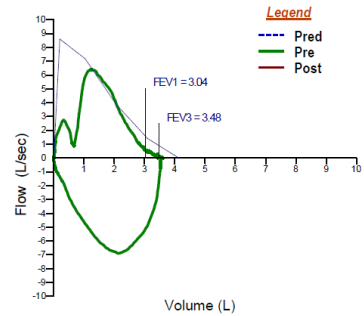

ATS ☒

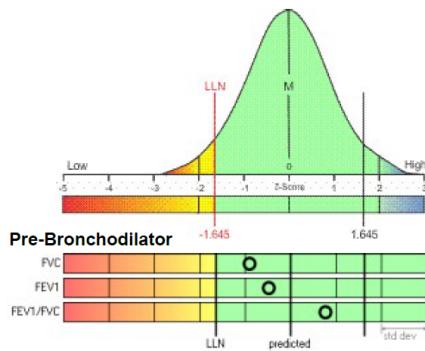

Pre-Bronchodilator



Summary of all Pre Efforts

	Pred	Best	%Prd	1	2	3	4	5	6	7	8
StartTime				20:13	20:17	20:14	---	---	---	---	---
FVC	L	4.14	3.61	87	3.33	3.61	3.42	---	---	---	---
FEV ₁	L	3.26	3.04	93	2.85	3.04	3.00	---	---	---	---
FEV ₁ / FVC	%	79	84	106	86	84	88	---	---	---	---
FET	sec	---	8.47		8.93	8.47	3.41	---	---	---	---
V [EXT]	L	---	0.66		0.44	0.66	0.51	---	---	---	---
V [EXT]/FVC	---	---	---		---	---	---	---	---	---	---
<input checked="" type="checkbox"/> Fails ATS due to:				Cough	Cough	Cough					




Meets ATS Effort




Meets ATS Reproducibility



FVC Flow vs. Volume

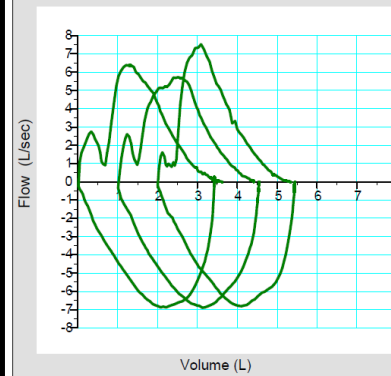

FVC Volume vs. Time

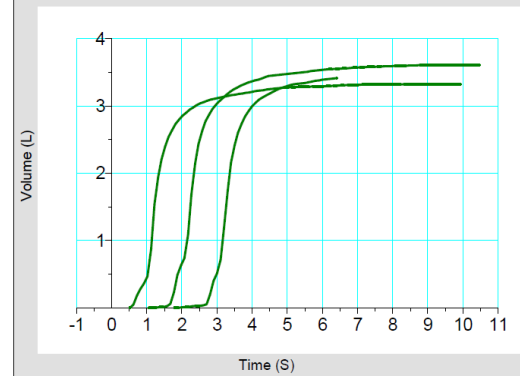

Hesitation; Slow Start; Large Extrapolated Volume
Delete Curve; Coach: Blast FASTER

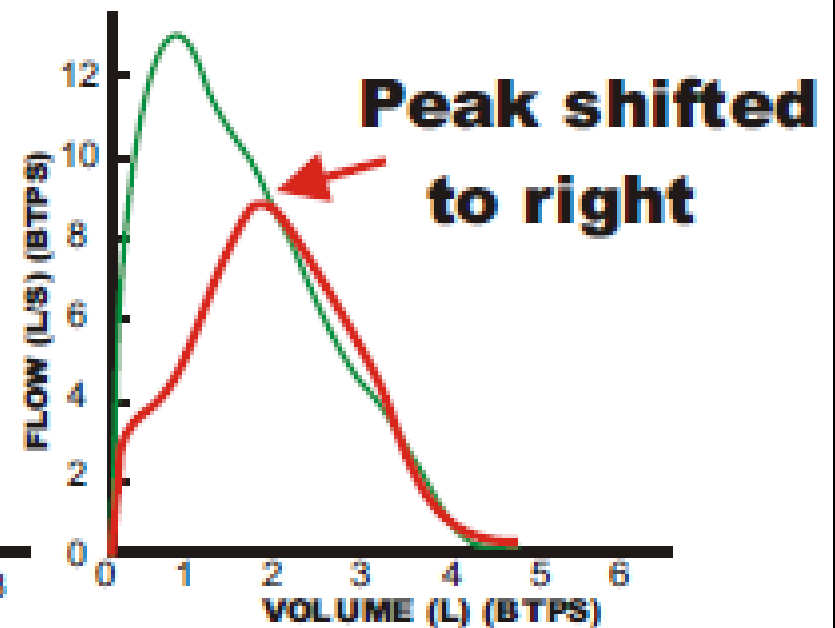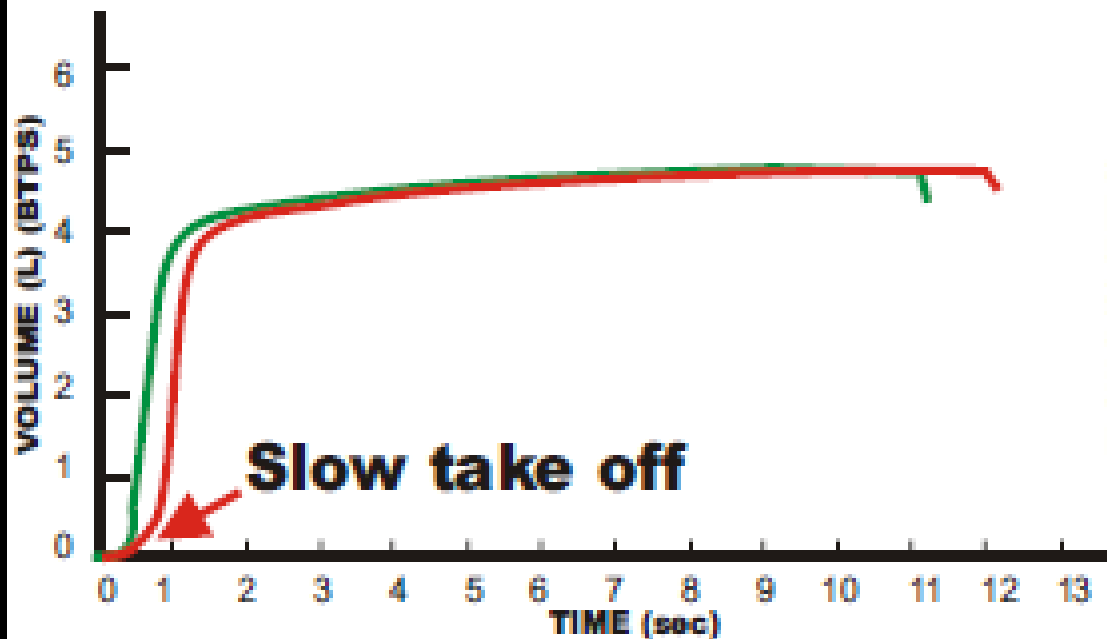



Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236




Phone: (210) 292-4278

Patient

Name: BMT Test ID: 10005 Test date/time: 2/17/2019 8:35:43 PM
Height at test: 66 in Sex: M Birthdate: 01-Jul-00 Age at test: 18
Weight at test: 155 lb
BMI at test: 25.1 Smoking history (pk-yrs): N/A Ethnicity: White
Physician: Doctor D. Doctor, M.D. Technician: James M. Quinn, MD
Predicted set: GLI 2012

Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.07	3.79	-3.00	66	
FEV ₁	L	2.60	3.26	-3.01	65	
FEV ₁ / FVC	%	85	75	-0.28	98	
FEF ₂₅₋₇₅ [ISO]	L/s	3.05	2.99		67	
PEFR	L/s	3.73	6.64		43	
FET	sec	6.65				

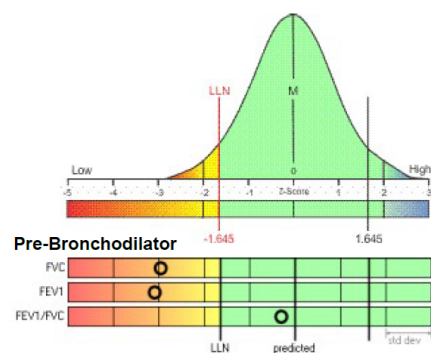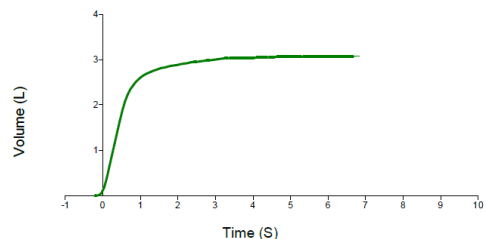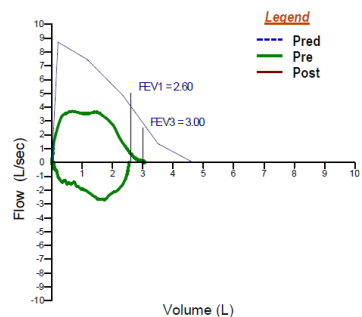


Summary of all Pre Efforts

	Pred	Best	%Prd	1	2	3	4	5	6	7	8
StartTime				20:40	20:37	20:39	---	---	---	---	---
FVC	L	4.67	3.07	66	3.07	3.53	2.88	---	---	---	---
FEV ₁	L	4.03	2.60	65	2.60	2.94	2.59	---	---	---	---
FEV ₁ / FVC	%	87	85	98	85	83	90	---	---	---	---
FET	sec	---	6.65		6.65	6.55	5.95	---	---	---	---
V [EXT]	L	---	0.12		0.12	0.29	0.10	---	---	---	---
V [EXT]/FVC	---	---	---		---	---	---	---	---	---	---


⊗ Fails ATS due to:

Cough Start of expiration



FVC Flow vs. Volume

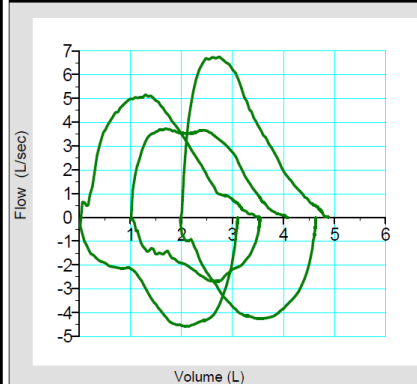

FVC Volume vs. Time


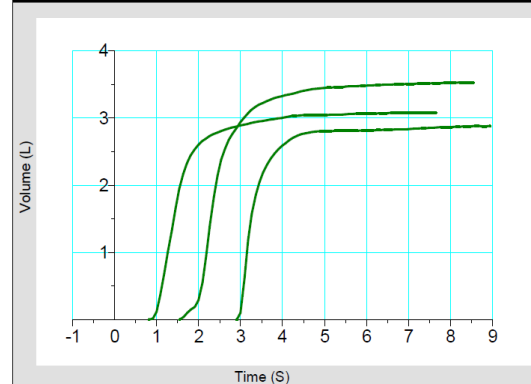


Poor Initial Blast
Coach: Blast air out HARDER

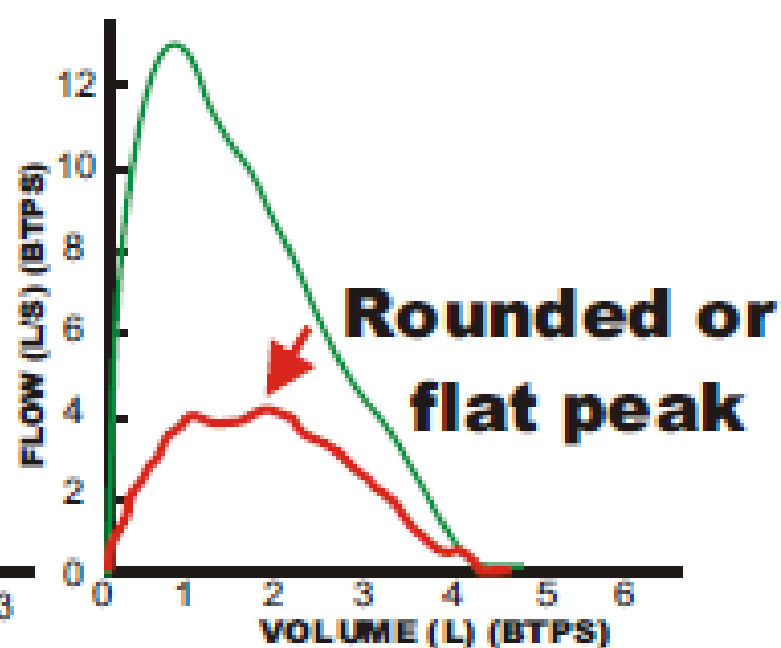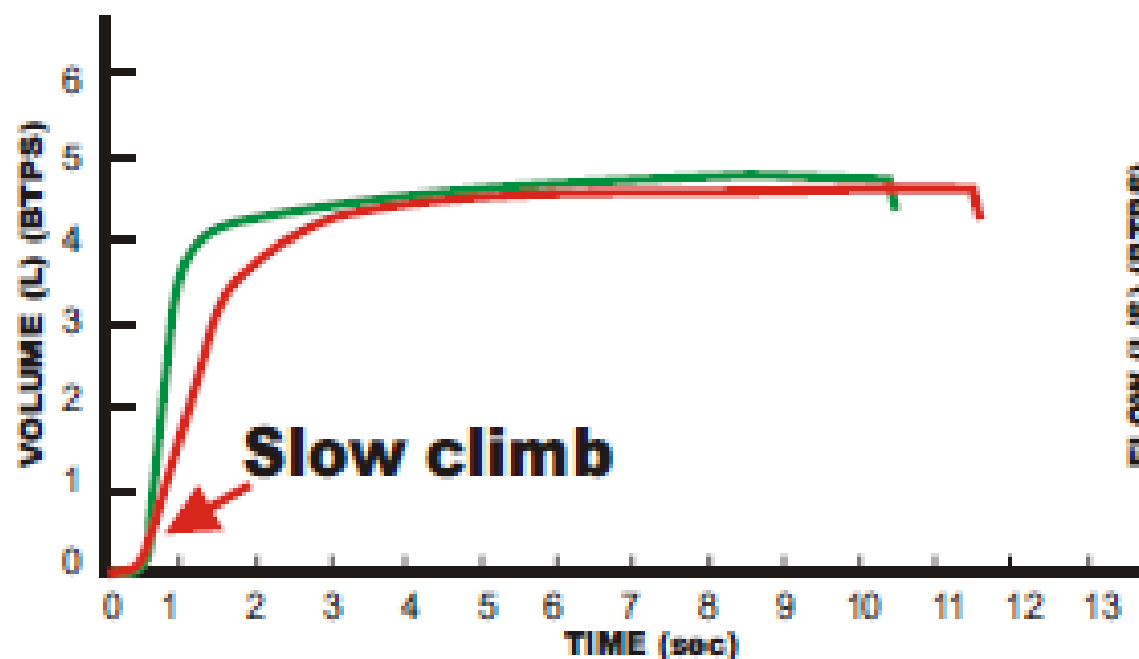

Incomplete Inhalation

Coach: Take a DEEPER breath

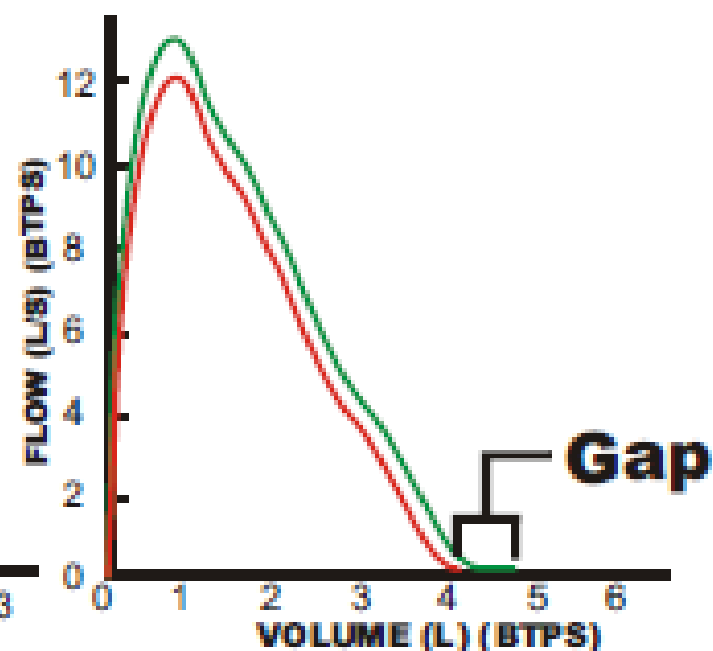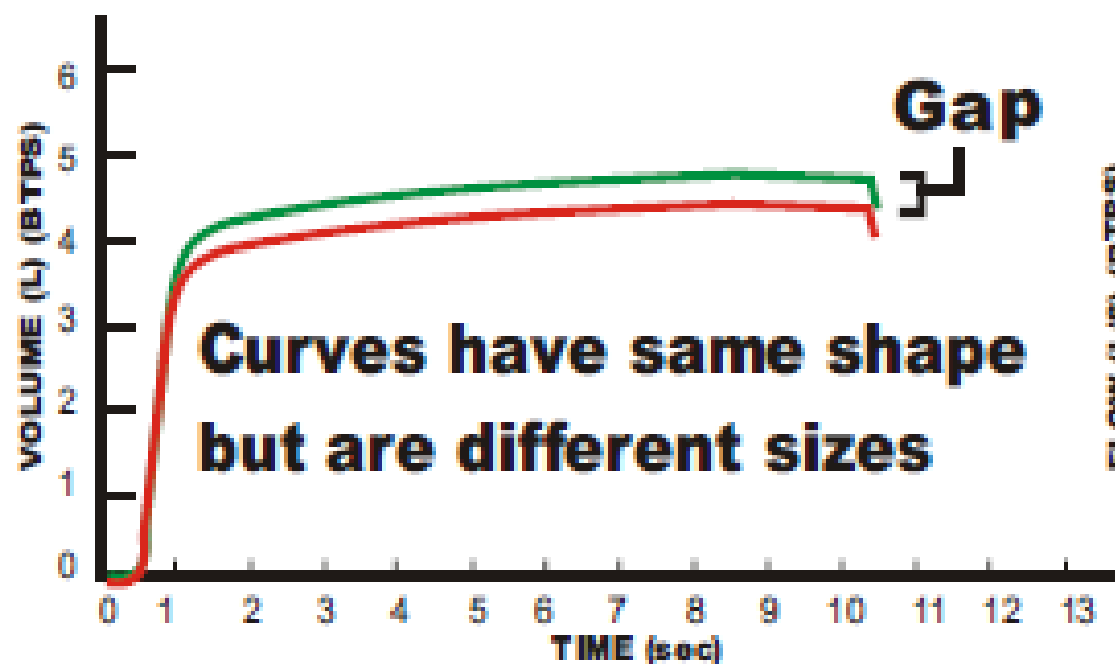



Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236

Phone: (210) 292-4278

Patient

Name: Pavifom Test

ID: 10004

Test date/time: 2/17/2019 8:28:02 PM

Height at test: 66 in

Sex: M

Birthdate: 01-Jul-62

Age at test: 56

Weight at test: 160 lb

Smoking history (pk-yrs): N/A

Ethnicity: White

BMI at test: 25.9




Physician: Doctor D. Doctor, M.D.

Technician: James M. Quinn, MD

Predicted set: GLI 2012

Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.50	3.18	-1.09	85	
FEV ₁	L	2.81	2.49	-0.97	86	
FEV ₁ / FVC	%	80	67	0.19	101	
FEF ₂₅₋₇₅ [ISO]	L/s	2.85	1.46		99	
PEFR	L/s	7.67	6.54		89	
FET	sec	9.70				

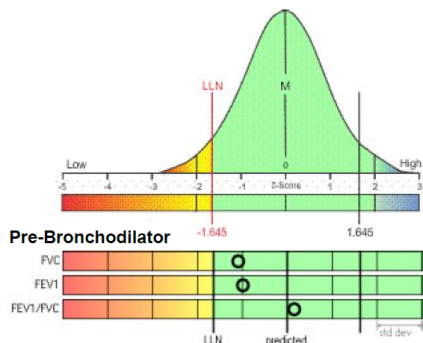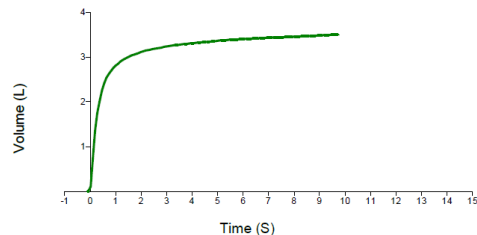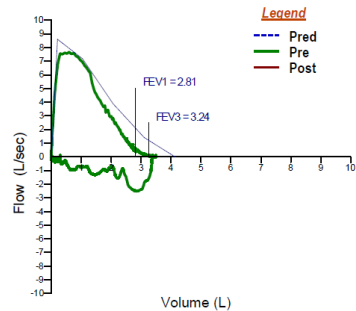


Summary of all Pre Efforts


	Pred	Best	%Prd	1	2	3	4	5	6	7	8
StartTime				20:28	20:28	20:29	---	---	---	---	---
FVC	L	4.14	3.50	85	3.50	3.47	3.40	---	---	---	---
FEV ₁	L	3.26	2.81	86	2.81	2.66	2.71	---	---	---	---
FEV ₁ / FVC	%	79	80	101	80	77	80	---	---	---	---
FET	sec	---	9.70		9.70	11.02	8.74	---	---	---	---
V [EXT]	L	---	0.07		0.07	0.07	0.06	---	---	---	---
V [EXT]/FVC	---	---	---		---	---	---	---	---	---	---

⊗ Fails ATS due to:

FVC Flow vs. Volume

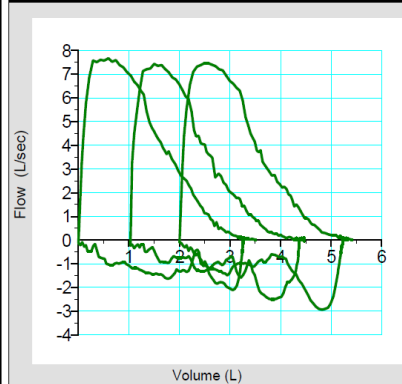

FVC Volume vs. Time

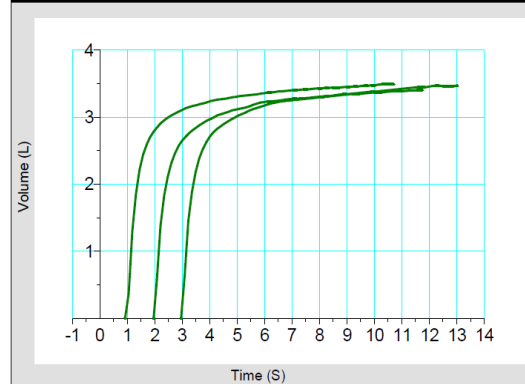

Clinical Data Gathered

- Forced Vital Capacity (FVC) maneuver
- Measurements
 - FVC = forced vital capacity
 - FEV_1 = forced expiratory volume in one second
 - Ratio FEV_1/FVC
 - FET = forced expiratory time
 - Not recommended 2017 but may use in 2019*
 - FEF_{25-75} = “midflows” = MMEF (Maximal Mid-Expiratory Flows)
 - PEFR = peak expiratory flow rate
 - New in 2019
 - FIVC

FVC

- Forced Vital Capacity
- Effort dependent
- Presentation*
 - Value in liters
 - Referenced lower limit of normal
 - Referenced Z score
 - Referenced % predicted (mean)
 - Do not present the predicted (mean) value

2017 ATS Reporting Standards

SPIROMETRY

	Pre-Bronchodilator				Post-Bronchodilator				
	Best	LLN	z-score	%Pred	Best	z-score	%Pred	Change	%Chng
FVC (L)	3.90	3.70	-1.34	82%					
FEV1 (L)	2.02	2.91	-3.78	54%					
FEV1/FVC	0.52	0.68	-3.54						
FET (s)	10.3								
Reference values: GLI 2012 Test quality: Pre: FEV1 - A, FVC - A; Post: FEV1 - A, FVC - B									

FEV₁

- Forced expiratory volume in one second
- Effort dependent
- Presentation*
 - Value in liters
 - Referenced lower limit of normal
 - Referenced Z score
 - Referenced % predicted (mean)
 - Do not present the predicted (mean) value

2017 ATS Reporting Standards

SPIROMETRY

	Pre-Bronchodilator				Post-Bronchodilator				
	Best	LLN	z-score	%Pred	Best	z-score	%Pred	Change	%Chng
FVC (L)	3.90	3.70	-1.34	82%					
FEV1 (L)	2.02	2.91	-3.78	54%					
FEV1/FVC	0.52	0.68	-3.54						
FET (s)	10.3								
Reference values: GLI 2012 Test quality: Pre: FEV1 - A, FVC - A; Post: FEV1 - A, FVC - B									

FEV₁/FVC Ratio

- Not an independent test - simply mathematical relationship
- Presentation*
 - Presented ONLY as an absolute ratio (ie 0.72)
 - Do not present as % (not 72%)
 - Referenced lower limit of normal
 - Referenced Z score
 - Definitely do not present as % predicted (mean)

2017 ATS Reporting Standards

SPIROMETRY

	Pre-Bronchodilator				Post-Bronchodilator				
	Best	LLN	z-score	%Pred	Best	z-score	%Pred	Change	%Chng
FVC (L)	3.90	3.70	-1.34	82%					
FEV1 (L)	2.02	2.91	-3.78	54%					
FEV1/FVC	0.52	0.68	-3.54						
FET (s)	10.3								
Reference values: GLI 2012 Test quality: Pre: FEV1 - A, FVC - A; Post: FEV1 - A, FVC - B									

FEV₁/FVC Ratio

- Key Factors
 - FEV₁/FVC ratio < lower limit of normal indicates and defines an obstructive pattern
 - Most sensitive measure of obstruction
- Severity of obstruction is determined by FEV₁

Midflows

- $FEF_{25-75\%}$
- MMEF = maximal mid expiratory flow rate
- 2017
 - Not recommended for use or in report*
 - Have not demonstrated added value for identifying obstruction in adults or children
- 2019
 - May be reported without endorsing it

Grading Adequacy

- Direct observation for proper effort
- Acceptability criteria – within each test/effort
- Reproducibility criteria – between tests/efforts

Grading Adequacy

- Acceptability
 - Examination of tracing and values within maneuver
 - A good start - no hesitation (extrapolated volume criteria available)
 - Sharp rise in peak flow
 - Rise from 10% to 90% PEF should be ≤ 150 milliseconds
 - Within first 25% of FVC (not ATS)
 - Flow/volume loop smooth without notching or artifact
 - No early cough
 - No early termination/glottic closure
 - Adequate duration when **end of forced expiration (EOFE) – not end of test (EOT)**
 - No change in volume (< 0.025 L) for > 1 second (plateau in VT curve)
 - Effort is **> 15 sec**
 - No minimum time (no longer ≥ 3 sec in children and ≥ 6 sec in adults)
 - **FIVC – FVC ≤ 0.100 L or 5% of FVC – whichever is greater**

Grading Adequacy

- Reproducibility
 - Comparison between maneuvers
 - 3 acceptable spirograms
 - FVC and FEV1 graded independently
 - 2 best FVC and FEV1 measures
 - Within 0.150 L of each other for > 6 yo
 - Within 0.100 L or 10% of largest FVC whichever greater for ≤ 6 yo

2017 Grading Adequacy

Table 1. Quality Categories for FVC or FEV₁ in Adults and Children

Grade	Criteria for Adults and Older Children and for Children Aged 2–6 Years
A	≥3 acceptable tests with repeatability within 0.150 L for age 2–6, 0.100 L, or 10% of highest value, whichever is greater
B	≥2 acceptable tests with repeatability within 0.150 L for age 2–6, 0.100 L, or 10% of highest value, whichever is greater
C	≥2 acceptable tests with repeatability within 0.200 L for age 2–6, 0.150 L, or 10% of highest value, whichever is greater
D	≥2 acceptable tests with repeatability within 0.250 L for age 2–6, 0.200 L, or 10% of highest value, whichever is greater
E	One acceptable test
F	No acceptable tests

- Clinically useful = Grades A, B, C
- Should not use = Grades D, E, F

2019 Grading Adequacy

Grade	Number of Measurements	Repeatability: Age >6 yr	Repeatability: Age ≤6 yr*
A	≥3 acceptable	Within 0.150 L	Within 0.100 L*
B	2 acceptable	Within 0.150 L	Within 0.100 L*
C	≥2 acceptable	Within 0.200 L	Within 0.150 L*
D	≥2 acceptable	Within 0.250 L	Within 0.200 L*
E	≥2 acceptable OR 1 acceptable	>0.250 L N/A	>0.200 L* N/A
U	0 acceptable AND ≥1 usable	N/A	N/A
F	0 acceptable and 0 usable	N/A	N/A

Definition of abbreviation: N/A = not applicable.

The repeatability grade is determined for the set of prebronchodilator maneuvers and the set of post-bronchodilator maneuvers separately. The repeatability criteria are applied to the differences between the two largest FVC values and the two largest FEV₁ values. Grade U indicates that only usable but not acceptable measurements were obtained. *Although some maneuvers may be acceptable or usable at grading levels lower than A, the overriding goal of the operator must be to always achieve the best possible testing quality for each patient.* Adapted from Reference 114.

*Or 10% of the highest value, whichever is greater; applies for age 6 years or younger only.

- Always strive for grade A
- Other results may still contain useful data

Assessment of Normal Values

- Comparison with “normal/healthy” subjects
- Anthropomorphically similar
 - Birth Sex
 - Age (years to one decimal place)
 - Height
 - Ethnicity – should include Caucasian, African American, NE Asian, SE Asian, Mixed or Other *
- All parameters from the same reference pool
 - Global Lung Function Initiative (GLI) – 2012 (Quanjer 2012) *

Eur Respir J 2005;26:948-68.

Am J Respir Crit Care Med 2017;196: 1463-1472.

Am J Respir Crit Care Med 2019;200:70-88.

Reference Pools

Edit Patient Information

Last name:	<input type="text" value="Test"/>	First name:	<input type="text" value="First"/>
ID:	<input type="text" value="123456"/>		
DOB:	<input type="text" value="01/01/1962"/>	Sex:	<input checked="" type="radio"/> Male <input type="radio"/> Female
Height:	<input type="text" value="66.0"/> <input type="radio"/> cm <input checked="" type="radio"/> in	Weight:	<input type="text" value="160.0"/> <input type="radio"/> kg <input checked="" type="radio"/> lb
Smoking history:	<input type="text"/> pk-yrs	Predicteds:	<input type="text" value="Quanjer GLI 2012"/>
Ethnic group:	<input checked="" type="radio"/> Caucasian <input type="radio"/> African-American <input type="radio"/> Mexican-American <input type="radio"/> Asian <input type="radio"/> NE Asian <input type="radio"/> SE Asian <input type="radio"/> Mixed		
	<input type="radio"/> Other: <input type="text"/>	Ethnic correction:	Pre-defined
Diagnosis:	<input type="text"/>	Group:	<input type="text"/>
Comments:	<input type="text"/>		

OK Cancel Help



Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236

Phone: (210) 292-4278

Patient

Name: Afamjz Nomogram ID: 307193 Test date/time: 2/17/2019 4:29:03 PM
Height at test: 70 in
Weight at test: 140 lb Sex: F Birthdate: 25-May-93 Age at test: 25
BMI at test: 20.1 Smoking history (pk-yr): N/A Ethnicity: White
Physician: Doctor D. Doctor, M.D. Technician: James M. Quinn, MD
Predicted set: GLI 2012



Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.49	3.73	-2.08	75	
FEV ₁	L	2.86	3.18	-2.30	72	
FEV ₁ / FVC	%	82	74	-0.55	96	
FEF ₂₅₋₇₅ [ISO]	L/s		2.80			
PEFR	L/s	6.73	5.88		85	
FET	sec					

Legend

--- Pred
— Pre
— Post

ATS ☒

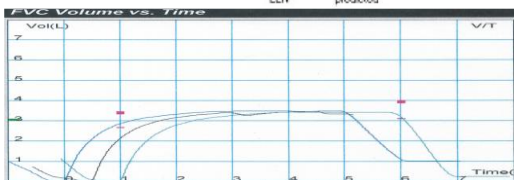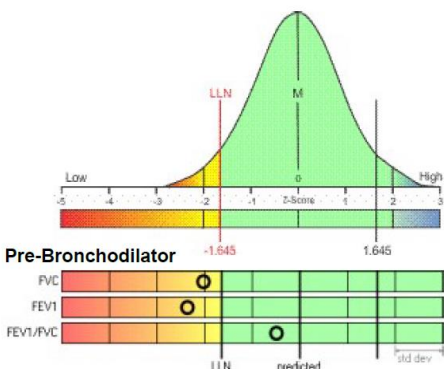

Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236

Phone: (210) 292-4278

Patient

Name: Afamjz Nomogram ID: 307193 Test date/time: 2/17/2019 4:29:03 PM
Height at test: 70 in
Weight at test: 140 lb Sex: F Birthdate: 25-May-93 Age at test: 25
BMI at test: 20.1 Smoking history (pk-yr): N/A Ethnicity: Black
Physician: Doctor D. Doctor, M.D. Technician: James M. Quinn, MD
Predicted set: GLI 2012





Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.49	3.13	-0.95	87	
FEV ₁	L	2.86	2.67	-1.22	84	
FEV ₁ / FVC	%	82	75	-0.63	95	
FEF ₂₅₋₇₅ [ISO]	L/s		2.23			
PEFR	L/s	6.73	5.54		85	
FET	sec					

Legend

--- Pred
— Pre
— Post

ATS ☒

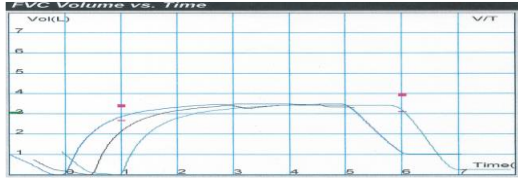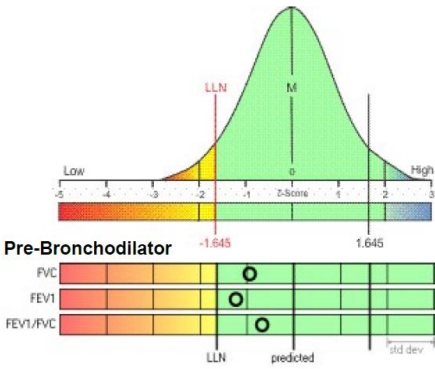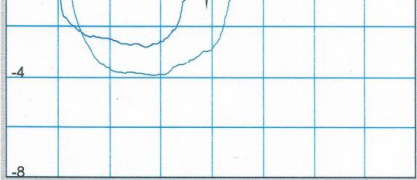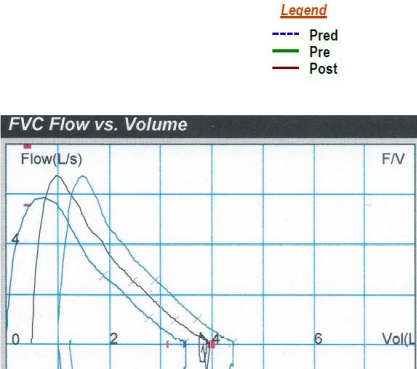



Allergy & Immunology Clinic
Wilford Hall Ambulatory Surgical Center
1100 Wilford Hall Loop
San Antonio, TX 78236 Phone: (210) 292-4278

Patient			
Name: Afamjz Nomogram	ID: 307193	Test date/time: 2/17/2019 4:29:03 PM	
Height at test: 70 in		Sex: F	Birthdate: 25-May-93
Weight at test: 140 lb			Age at test: 25
BMI at test: 20.1		Smoking history (pk-yrs): N/A	Ethnicity: White
Physician: Doctor D. Doctor, M.D.			Technician: James M. Quinn, MD
Predicted set: GLI 2012			


Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.49	3.73	-2.08	75	
FEV ₁	L	2.86	3.18	-2.30	72	
FEV ₁ / FVC	%	82	74	-0.55	96	
FEF ₂₅₋₇₅ [ISO]	L/s		2.80			
PEFR	L/s	6.73	5.88		85	
FET	sec					



Legend

--- Pred
--- Pre
--- Post

ATS

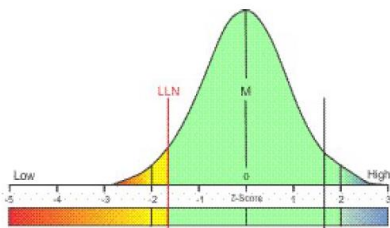

Pre-Bronchodilator

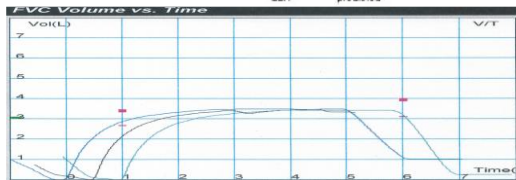

Allergy & Immunology Clinic
Wilford Hall Ambulatory Surgical Center
1100 Wilford Hall Loop
San Antonio, TX 78236 Phone: (210) 292-4278

Patient			
Name: Afamjz Nomogram	ID: 307193	Test date/time: 2/17/2019 4:29:03 PM	
Height at test: 70 in		Sex: F	Birthdate: 25-May-93
Weight at test: 140 lb			Age at test: 25
BMI at test: 20.1		Smoking history (pk-yrs): N/A	Ethnicity: Black
Physician: Doctor D. Doctor, M.D.			Technician: James M. Quinn, MD
Predicted set: GLI 2012			


Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.49	3.13	-0.95	87	
FEV ₁	L	2.86	2.67	-1.22	84	
FEV ₁ / FVC	%	82	75	-0.63	95	
FEF ₂₅₋₇₅ [ISO]	L/s		2.23			
PEFR	L/s	6.73	5.54		85	
FET	sec					



Legend

--- Pred
--- Pre
--- Post

ATS

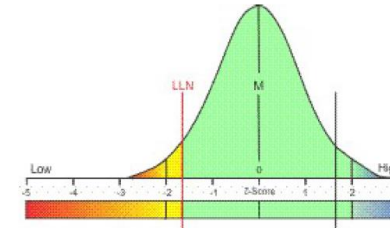

Pre-Bronchodilator

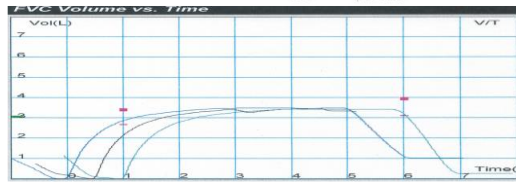



Allergy & Immunology Clinic
Wilford Hall Ambulatory Surgical Center
1100 Wilford Hall Loop
San Antonio, TX 78236 Phone: (210) 292-4278

Patient
Name: Afamjz Nomogram ID: 307193 Test date/time: 2/17/2019 4:29:03 PM
Height at test: 70 in
Weight at test: 140 lb Sex: F Birthdate: 25-May-93 Age at test: 25
BMI at test: 20.1 Smoking history (pk-yrs): N/A Ethnicity: White
Physician: Doctor D. Doctor, M.D. Technician: James M. Quinn, MD
Predicted set: GLI 2012



Spirometry

Parameter	Units	Best	ATS			Pos
			LLN	Z-score	% Pred	
FVC	L	3.49	3.73	-2.08	75	
FEV ₁	L	2.86	3.18	-2.30	72	
FEV ₁ / FVC	%	82	74	-0.55	96	
FEF ₂₅₋₇₅ [ISO]	L/s		2.80			
PEFR	L/s	6.73	5.88		85	
FET	sec					


Legend

--- Pred
— Pre
— Post

FVC Flow vs. Volume

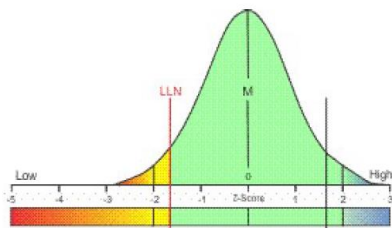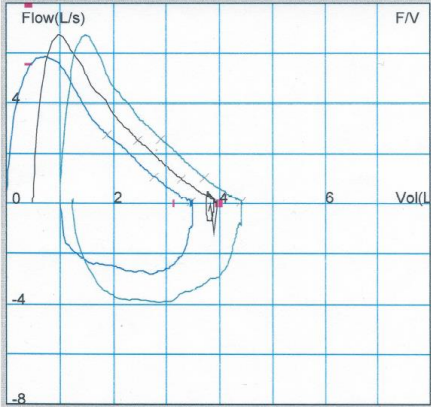

Pre-Bronchodilator



Allergy & Immunology Clinic
Wilford Hall Ambulatory Surgical Center
1100 Wilford Hall Loop
San Antonio, TX 78236 Phone: (210) 292-4278

Patient
Name: Afamjz Nomogram ID: 307193 Test date/time: 2/17/2019 4:29:03 PM
Height at test: 70 in
Weight at test: 140 lb Sex: F Birthdate: 25-May-93 Age at test: 25
BMI at test: 20.1 Smoking history (pk-yrs): N/A Ethnicity: Black
Physician: Doctor D. Doctor, M.D. Technician: James M. Quinn, MD
Predicted set: GLI 2012



Spirometry

Parameter	Units	Best	ATS			Pos
			LLN	Z-score	% Pred	
FVC	L	3.49	3.13	-0.95	87	
FEV ₁	L	2.86	2.67	-1.22	84	
FEV ₁ / FVC	%	82	75	-0.63	95	
FEF ₂₅₋₇₅ [ISO]	L/s		2.23			
PEFR	L/s	6.73	5.54		85	
FET	sec					



Legend

--- Pred
— Pre
— Post

FVC Flow vs. Volume

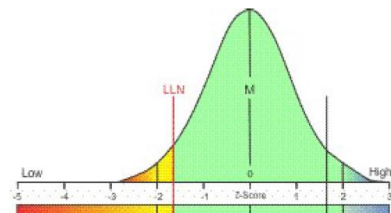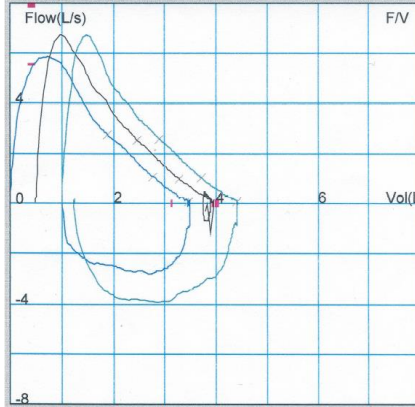

Pre-Bronchodilator

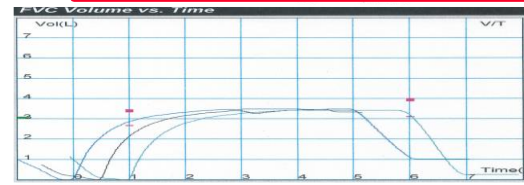



Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236

Phone: (210) 292-4278

Patient

Name: Asian Nomogram

ID: 305704

Test date/time: 2/16/2019 5:22:23 PM

Height at test: 70 in

Weight at test: 215 lb

BMI at test: 30.9

Physician: James M. Quinn, M.D.

Predicted set: GLI 2012

Sex: M

Birth date: 18 Dec 61

Age at test: 57

Smoking history (pk-yr): N/A

Ethnicity: White



Technician: James M. Quinn, MD

Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.52	3.65	-1.84	74	
FEV ₁	L	2.62	2.81	-2.00	71	
FEV ₁ / FVC	%	74	66	-0.59	95	
FEF ₂₅₋₇₅ [ISO]	L/s		1.59			
PEFR	L/s	5.95	7.12		63	
FET	sec					

Legend

Pred
Pre
Post

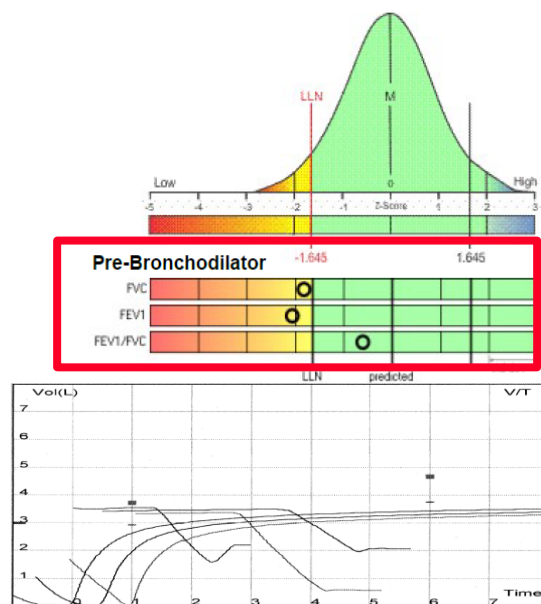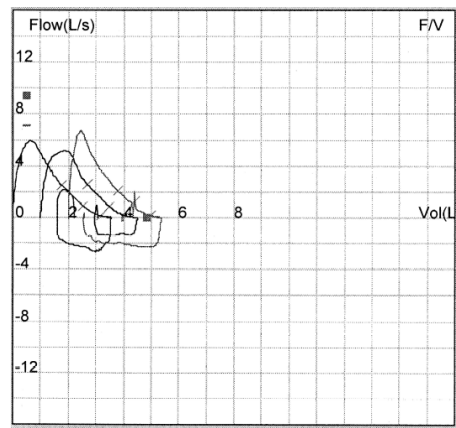

Allergy & Immunology Clinic

Wilford Hall Ambulatory Surgical Center

1100 Wilford Hall Loop

San Antonio, TX 78236

Phone: (210) 292-4278

Patient

Name: Asian Nomogram

ID: 305704

Test date/time: 2/16/2019 5:22:23 PM

Height at test: 70 in

Weight at test: 215 lb

BMI at test: 30.9

Physician: James M. Quinn, M.D.

Predicted set: GLI 2012

Sex: M

Birth date: 18 Dec 61

Age at test: 57

Smoking history (pk-yr): N/A

Ethnicity: Southeast Asian



Technician: James M. Quinn, MD

Spirometry

Parameter	Units	Best	LLN	Z-score	% Pred	Pos
FVC	L	3.52	3.21	-1.14	83	
FEV ₁	L	2.62	2.55	-1.51	78	
FEV ₁ / FVC	%	74	70	-1.02	92	
FEF ₂₅₋₇₅ [ISO]	L/s		1.71			
PEFR	L/s	5.95	7.12		63	
FET	sec					

Legend

Pred
Pre
Post



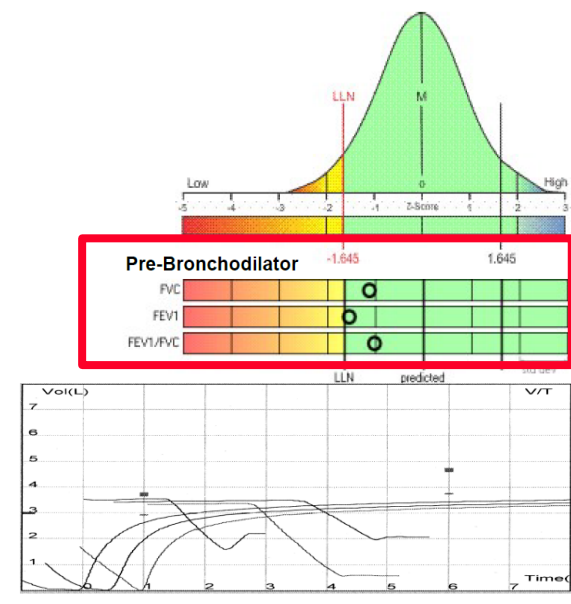
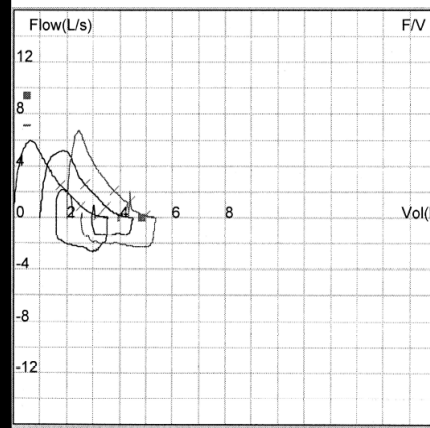


2017 ATS Reporting Standards

SPIROMETRY

	Pre-Bronchodilator				Post-Bronchodilator				
	Best	LLN	z-score	%Pred	Best	z-score	%Pred	Change	%Chng
FVC (L)	3.90	3.70	-1.34	82%	4.70	-0.09	99%	600 mL	20%
FEV ₁ (L)	2.02	2.91	-3.78	54%	2.61	-2.21	70%	590 mL	29%
FEV ₁ /FVC	0.52	0.68	-3.54		0.55	-3.35			
FET (s)	10.3				11.2				

Reference values: GLI 2012 Test quality: Pre: FEV₁ - A, FVC - A; Post: FEV₁ - A, FVC - B

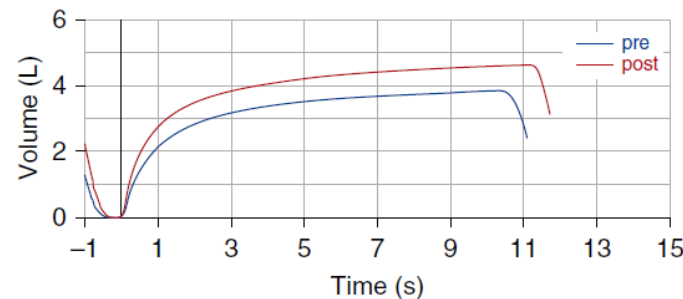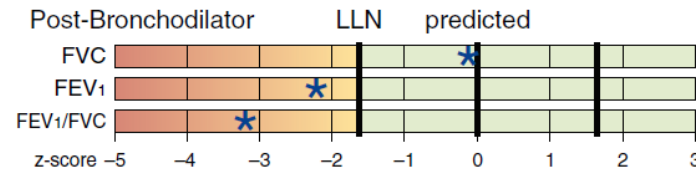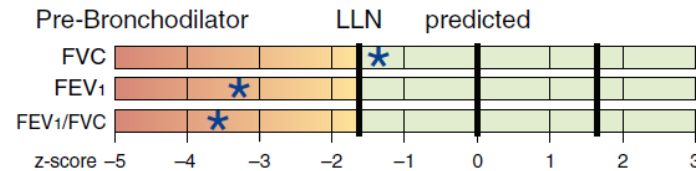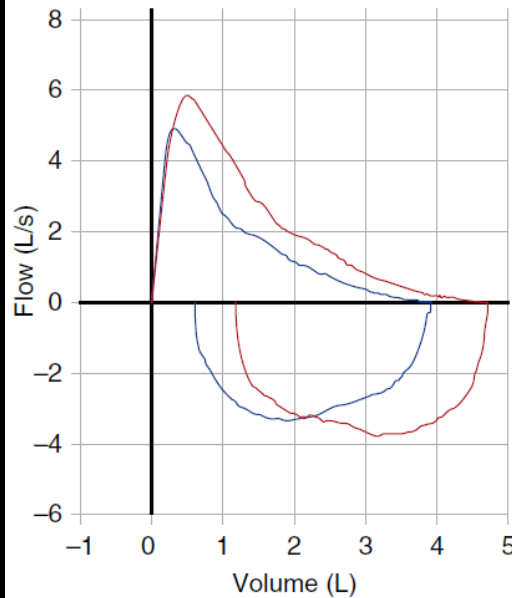





2017 ATS Reporting Standards

SPIROMETRY

	Pre-Bronchodilator					Post-Bronchodilator				
	Best	LLN	z-score	%Pred		Best	z-score	%Pred	Change	%Chng
FVC (L)	3.90	3.70	-1.34	82%		4.70	-0.09	99%	600 mL	20%
FEV1 (L)	2.02	2.91	-3.78	54%		2.61	-2.21	70%	590 mL	29%
FEV1/FVC	0.52	0.68	-3.54			0.55	-3.35			
FET (s)	10.3					11.2				
Reference values: GLI 2012 Test quality: Pre: FEV1 - A, FVC - A; Post: FEV1 - A, FVC - B										

2017 ATS Reporting Standards

Am J Respir Crit Care Med 2017;196: 1463-1472.

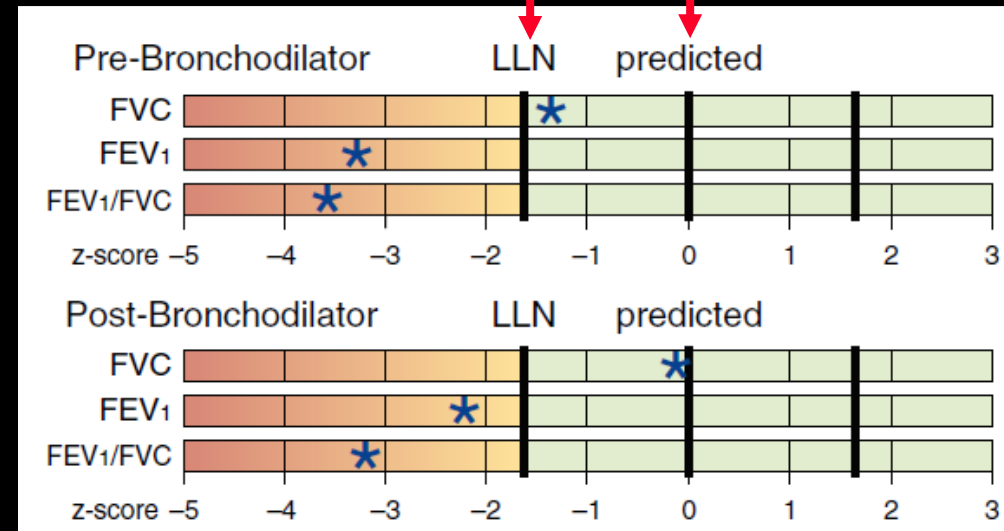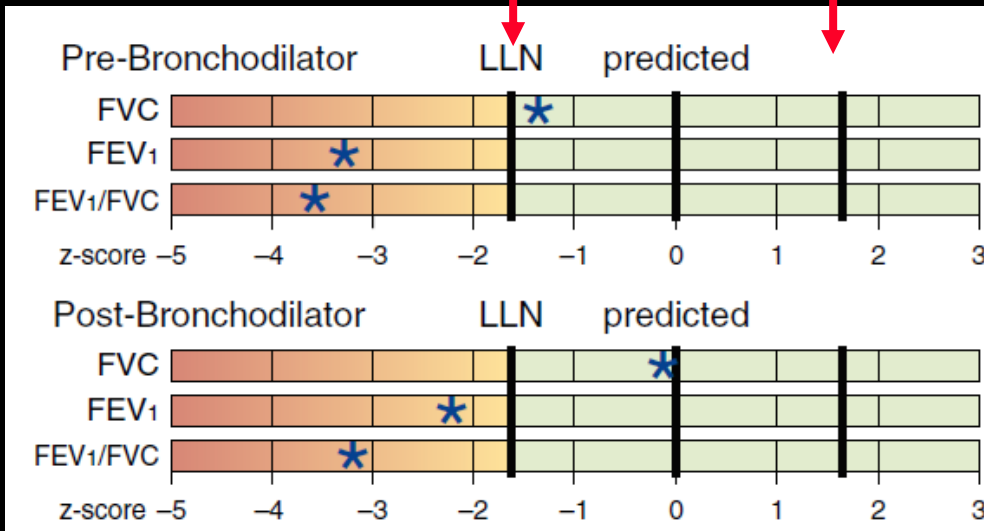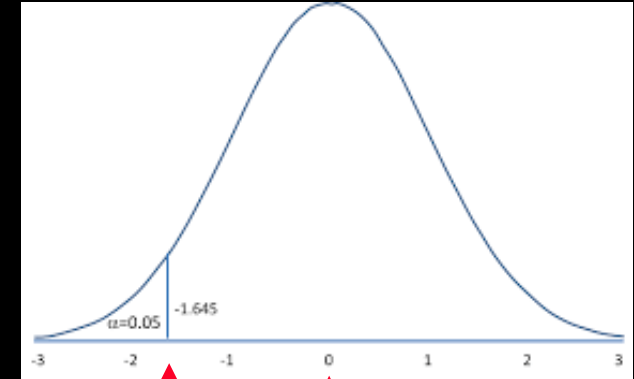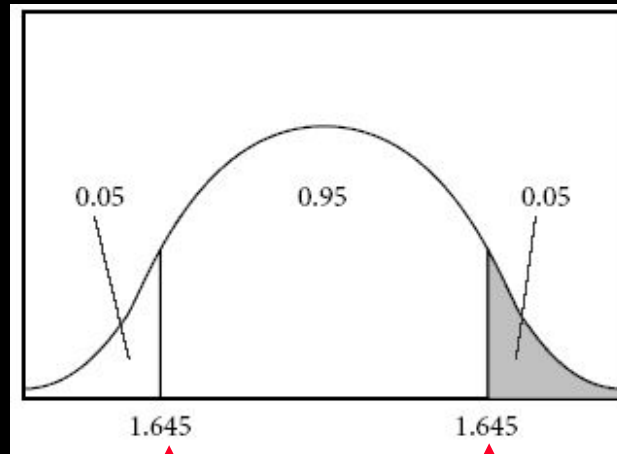

2017 ATS Reporting Standards

